


Technician: NS
Test ind: CP

P-R-T axes 69 -6 64

Handwritten signature

Unconfirmed

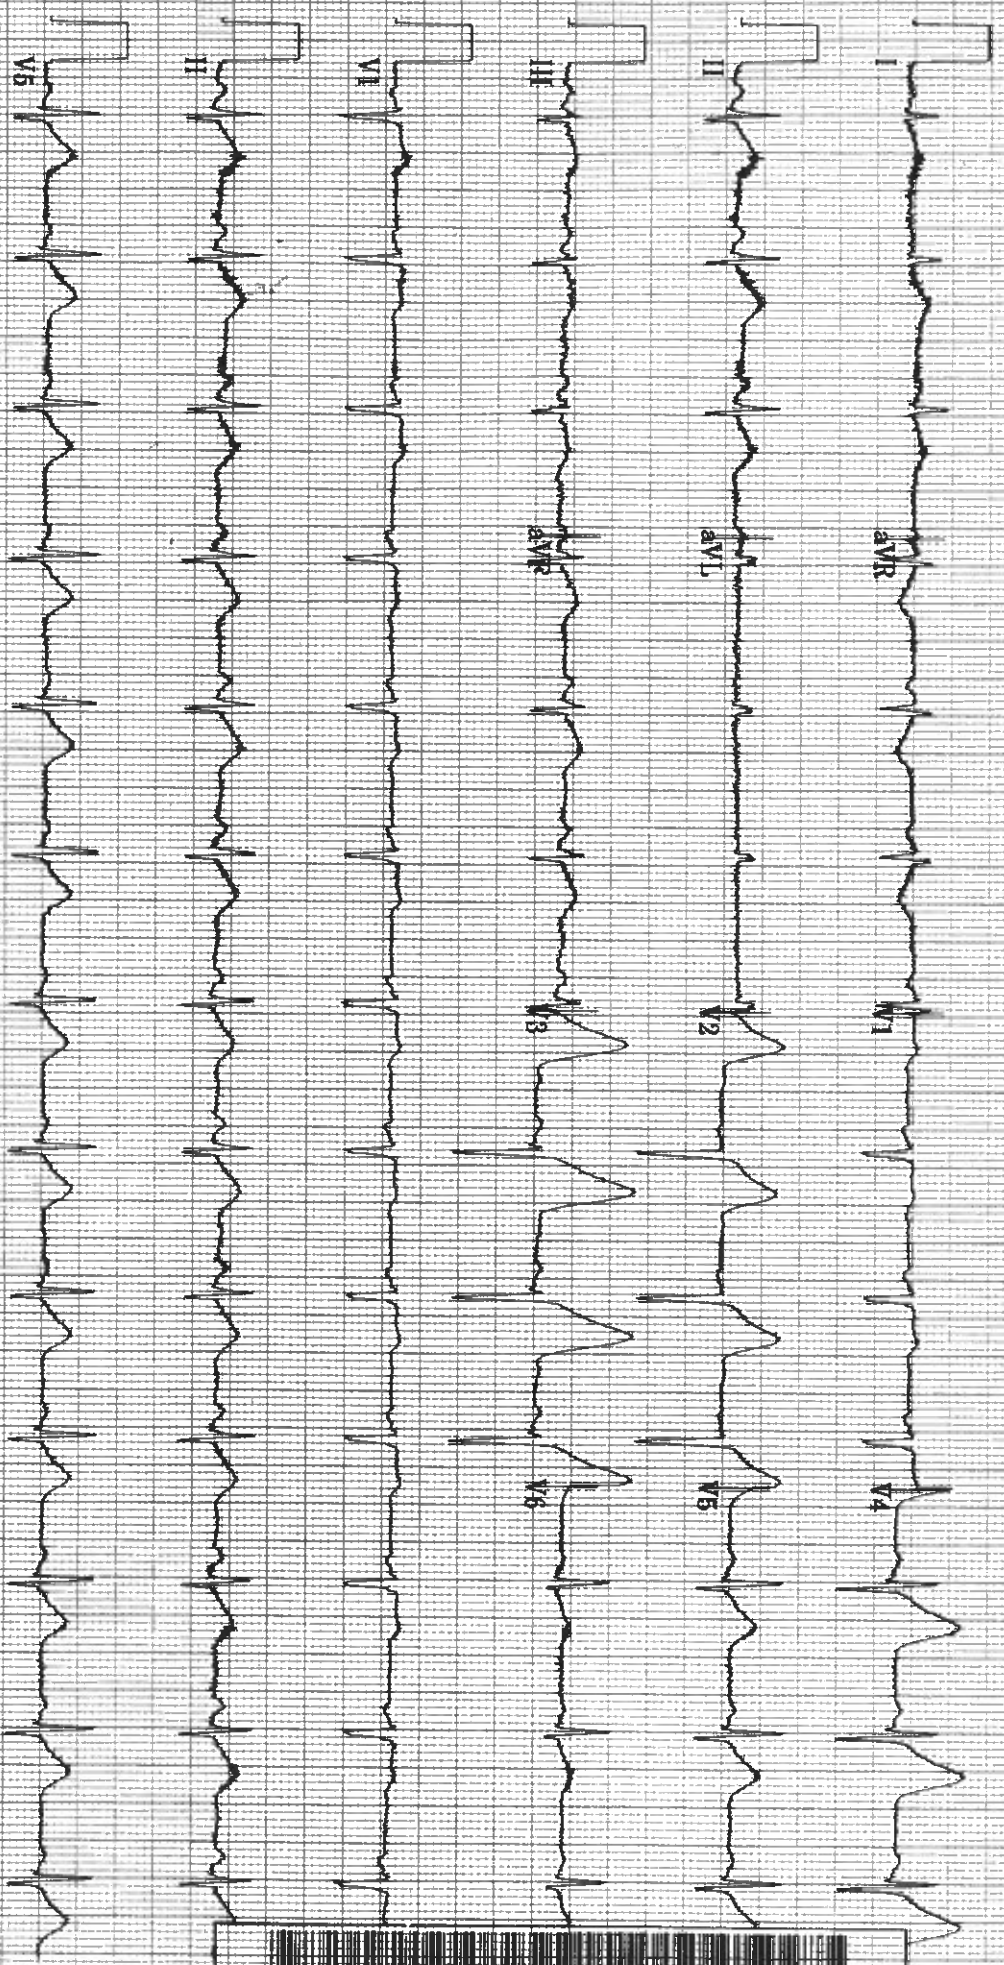

150 Hz 25.0 mm/s 10.0 mm/mV

4 by 2.5s + 3 rhythm 1ds

MAC55 0108

12SL™ 1241

COVIDIEN Kendall

Printed in USA

2366

